

FIG. 2 is a cross-sectional view of the device of FIG. 1, taken along line 2-2 of FIG. 1, showing the device in a contracted state. The device is shown in a contracted state, with the outer sheath 10 and the inner sheath 12 being pulled together to form a single layer. The device is shown in a contracted state, with the outer sheath 10 and the inner sheath 12 being pulled together to form a single layer. The device is shown in a contracted state, with the outer sheath 10 and the inner sheath 12 being pulled together to form a single layer.

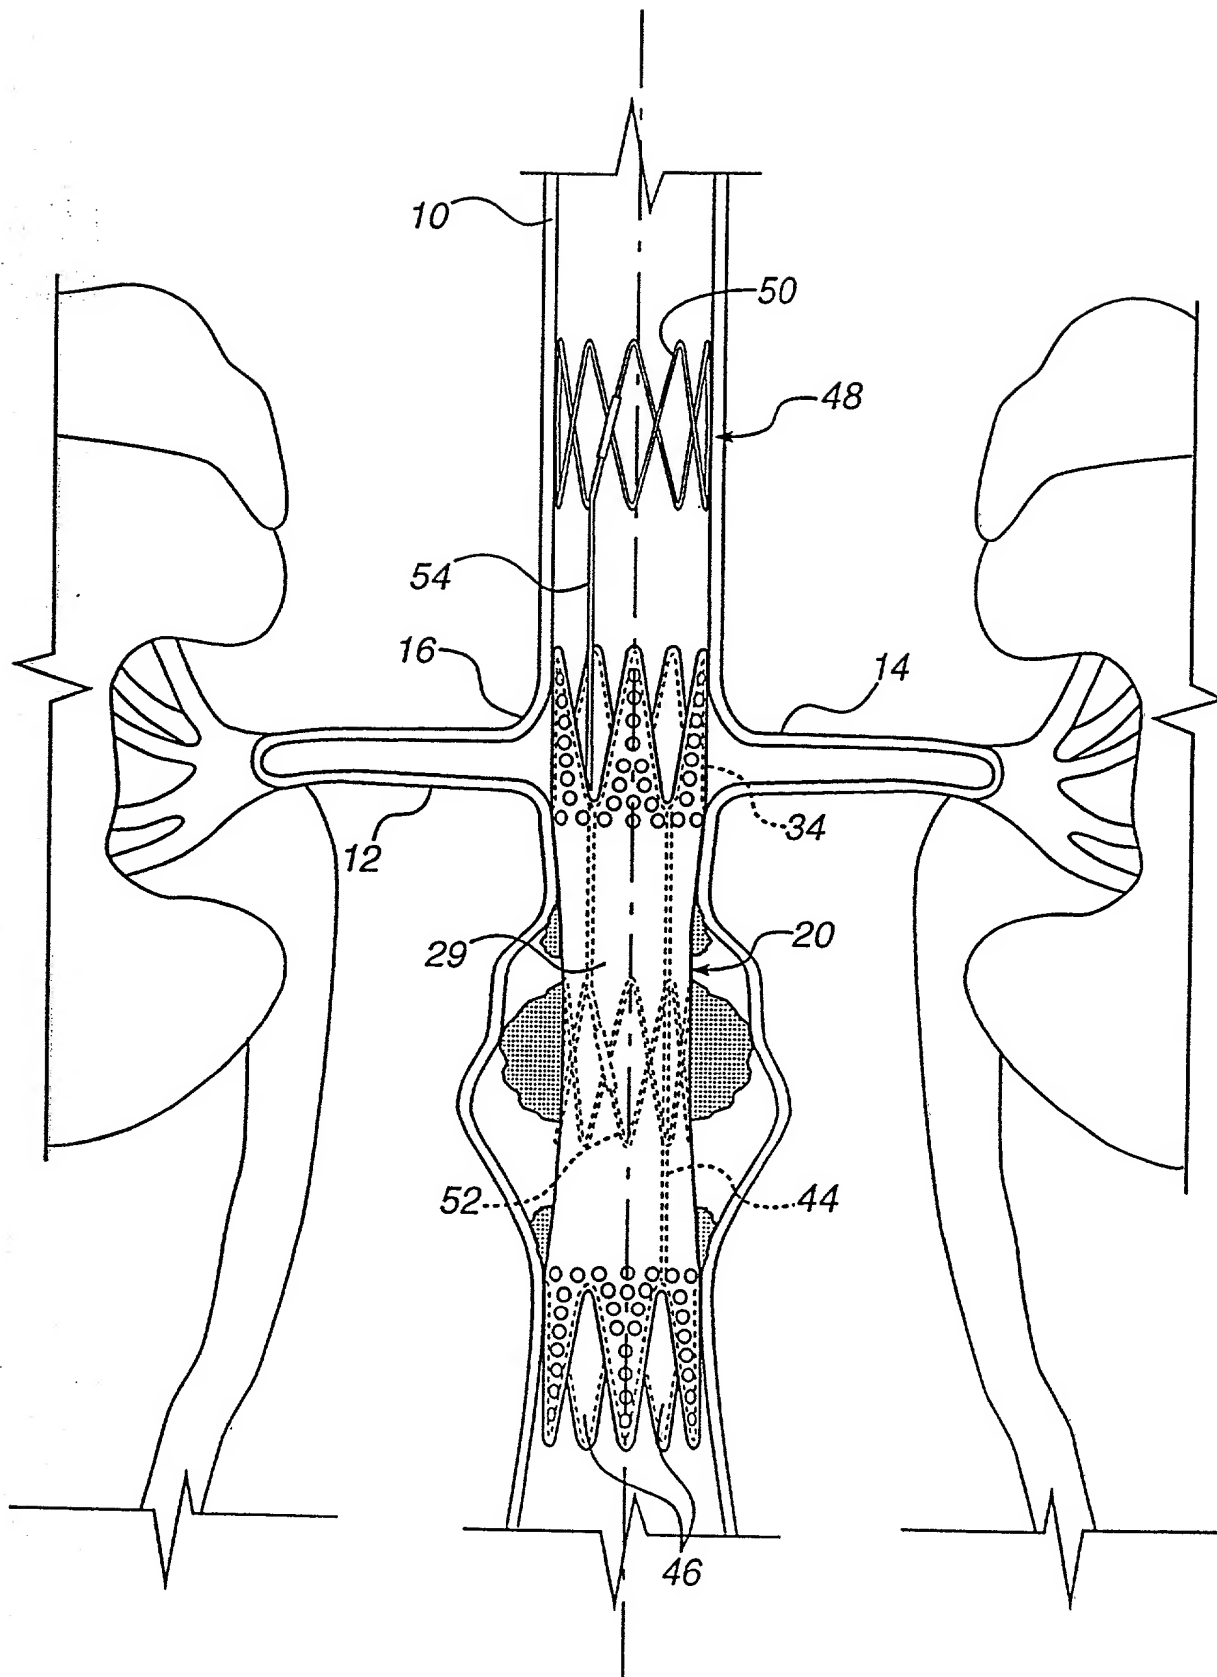


FIG. 2



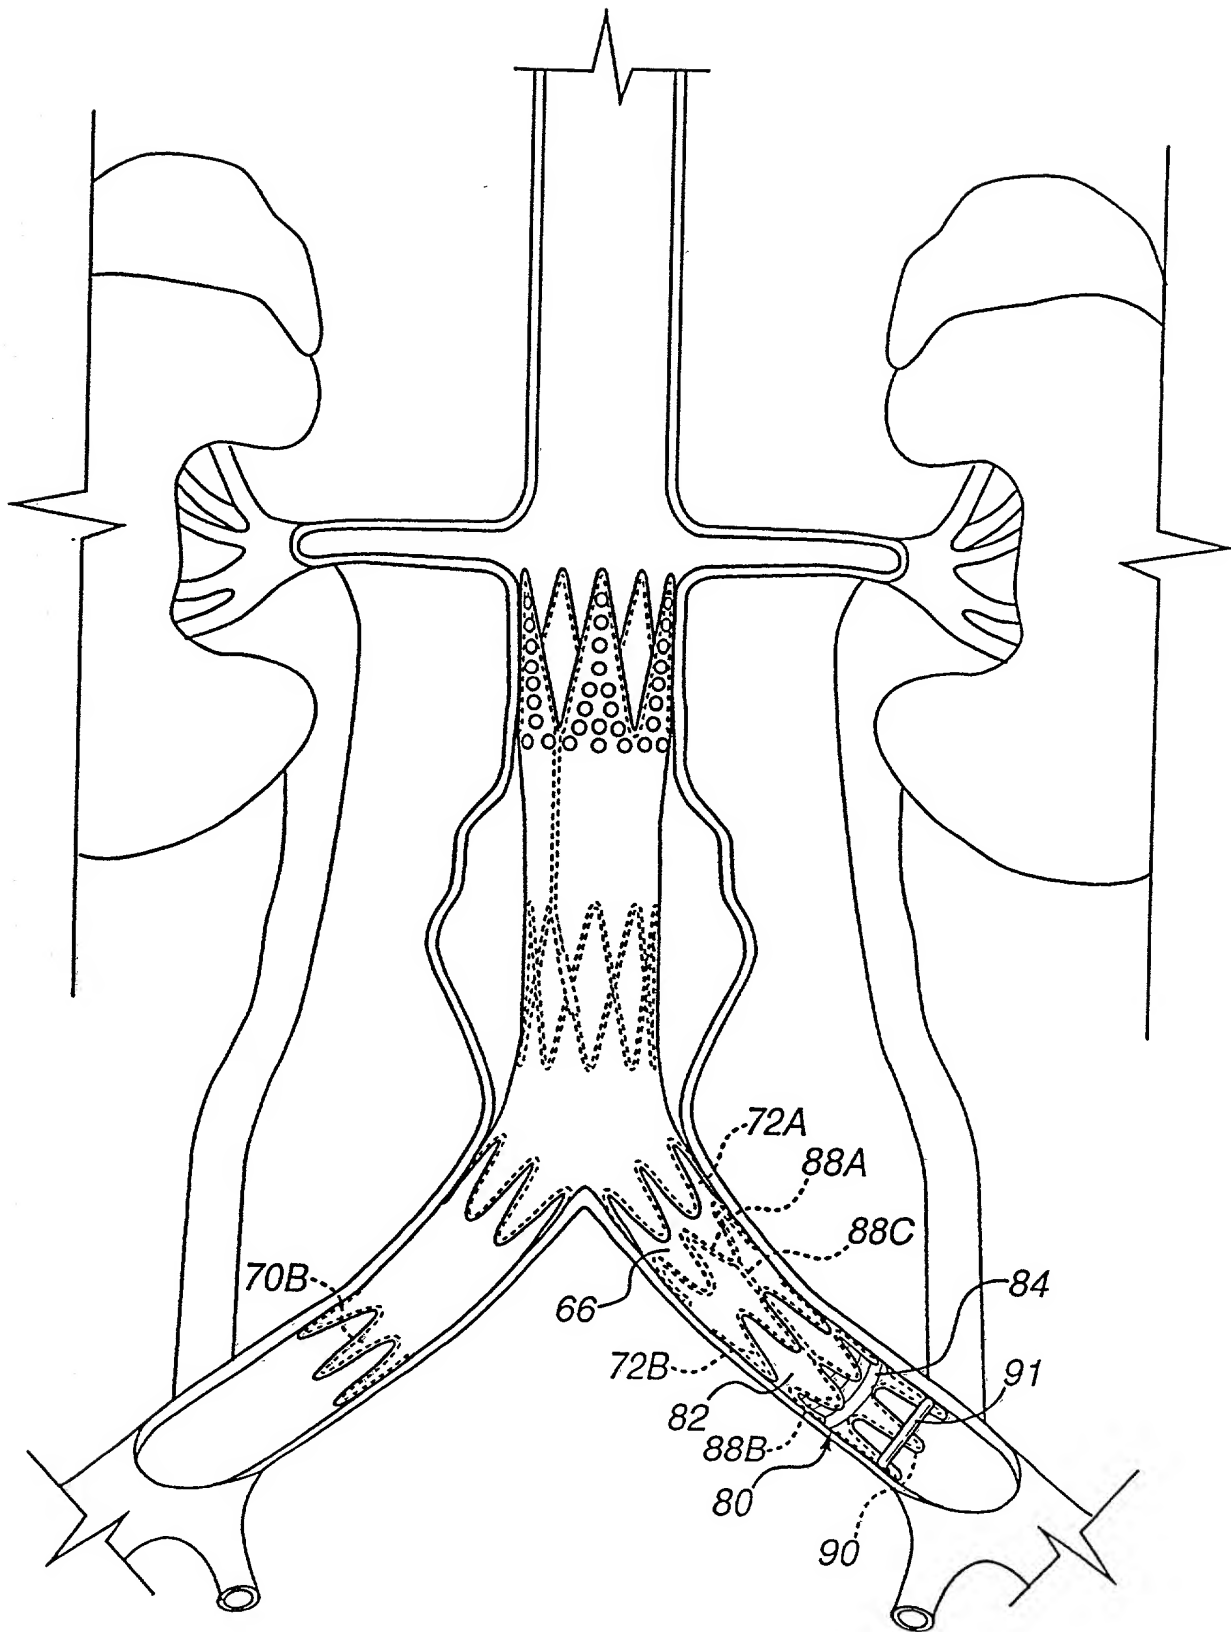


FIG. 4

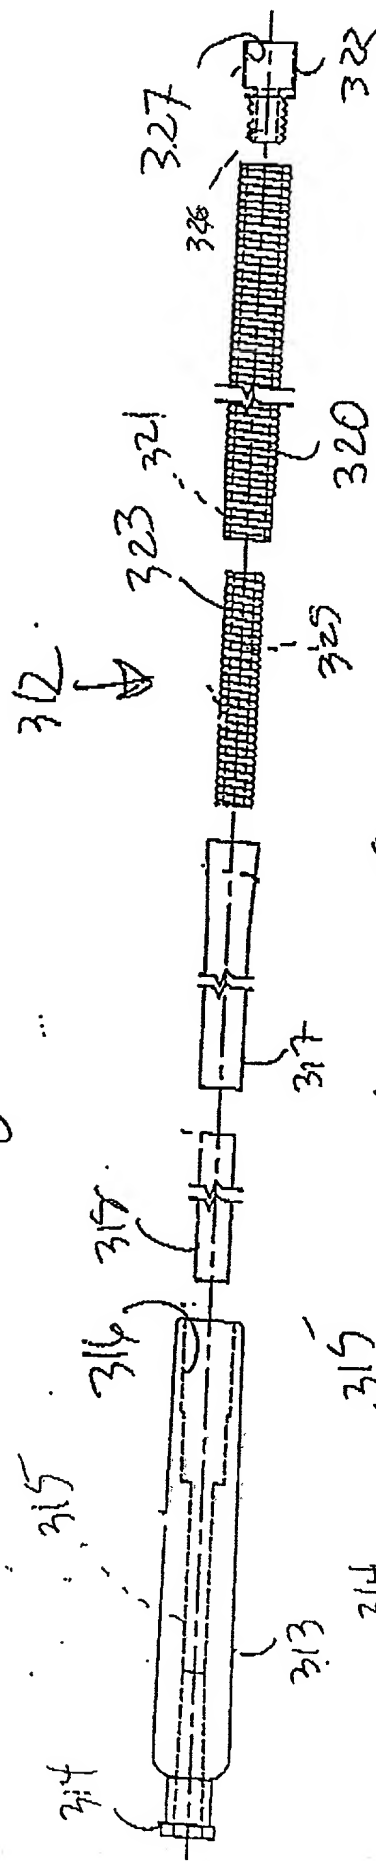

SA
F-1

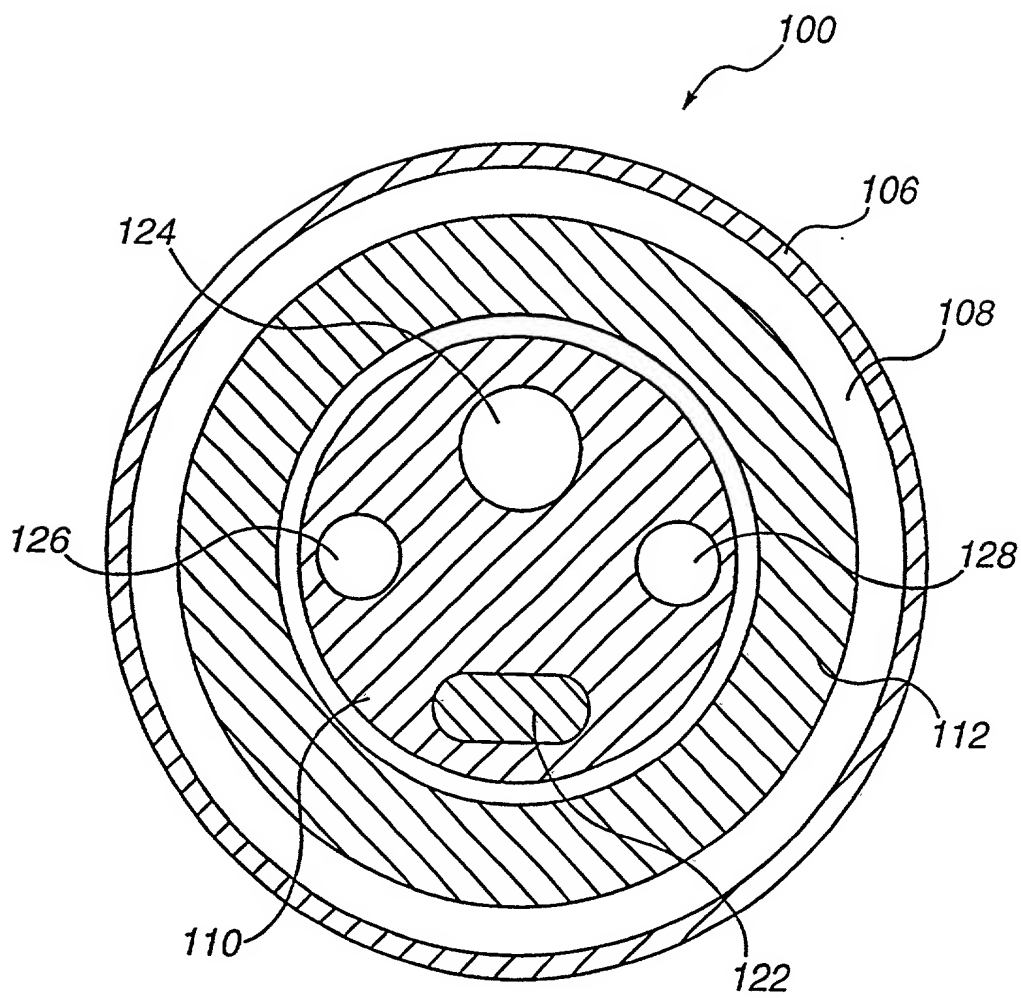


Fig. 6

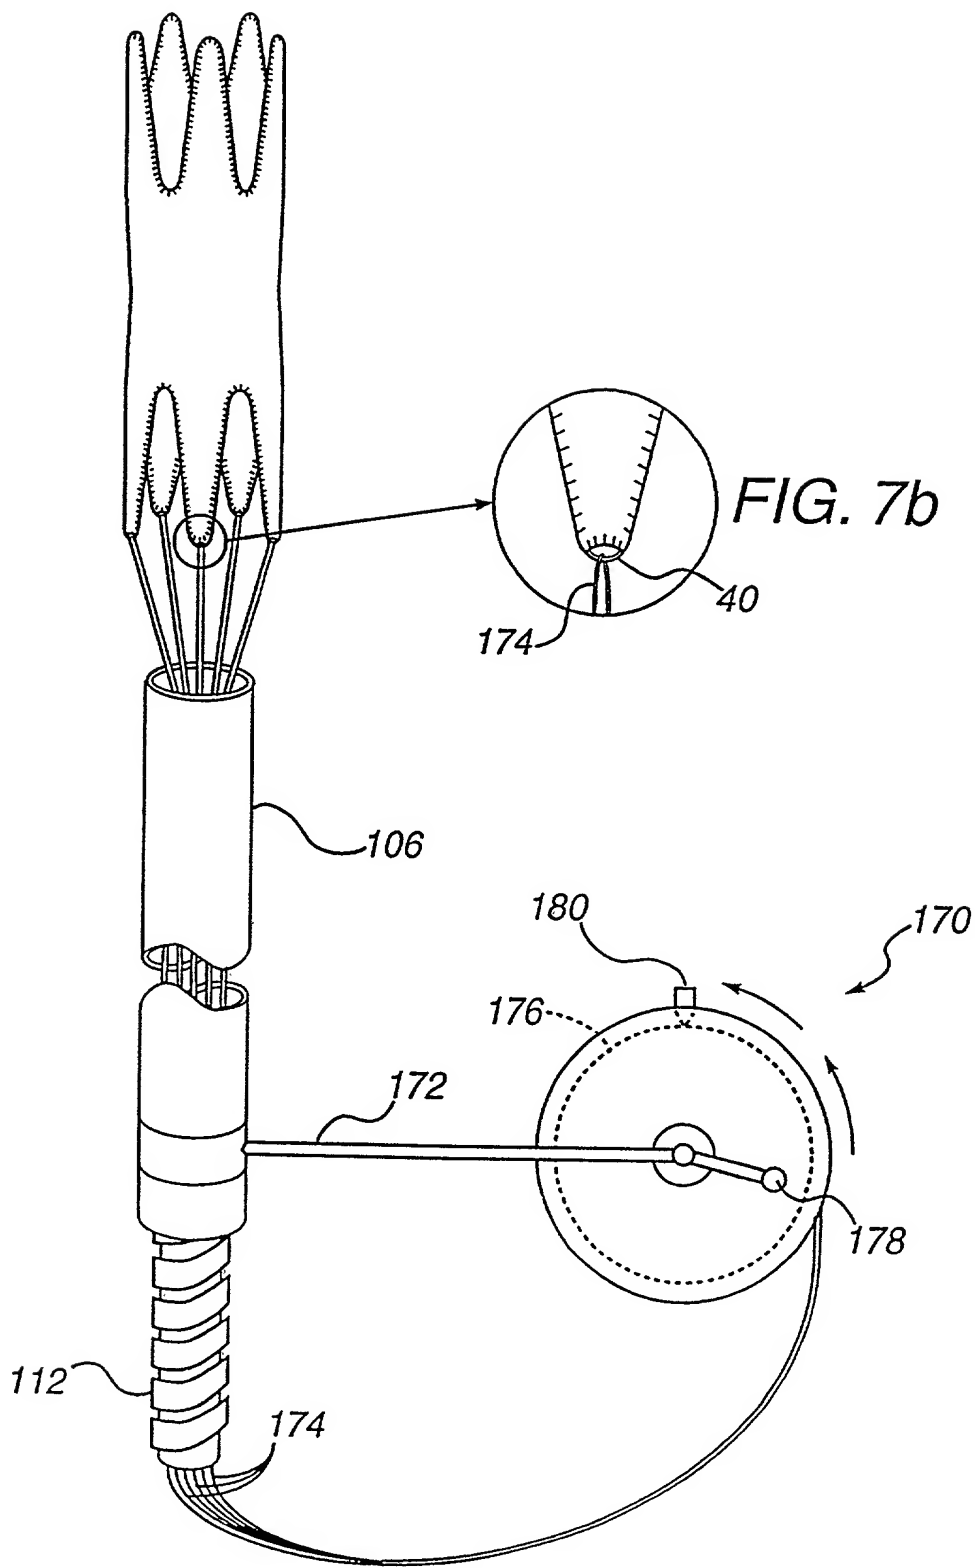


FIG. 7a

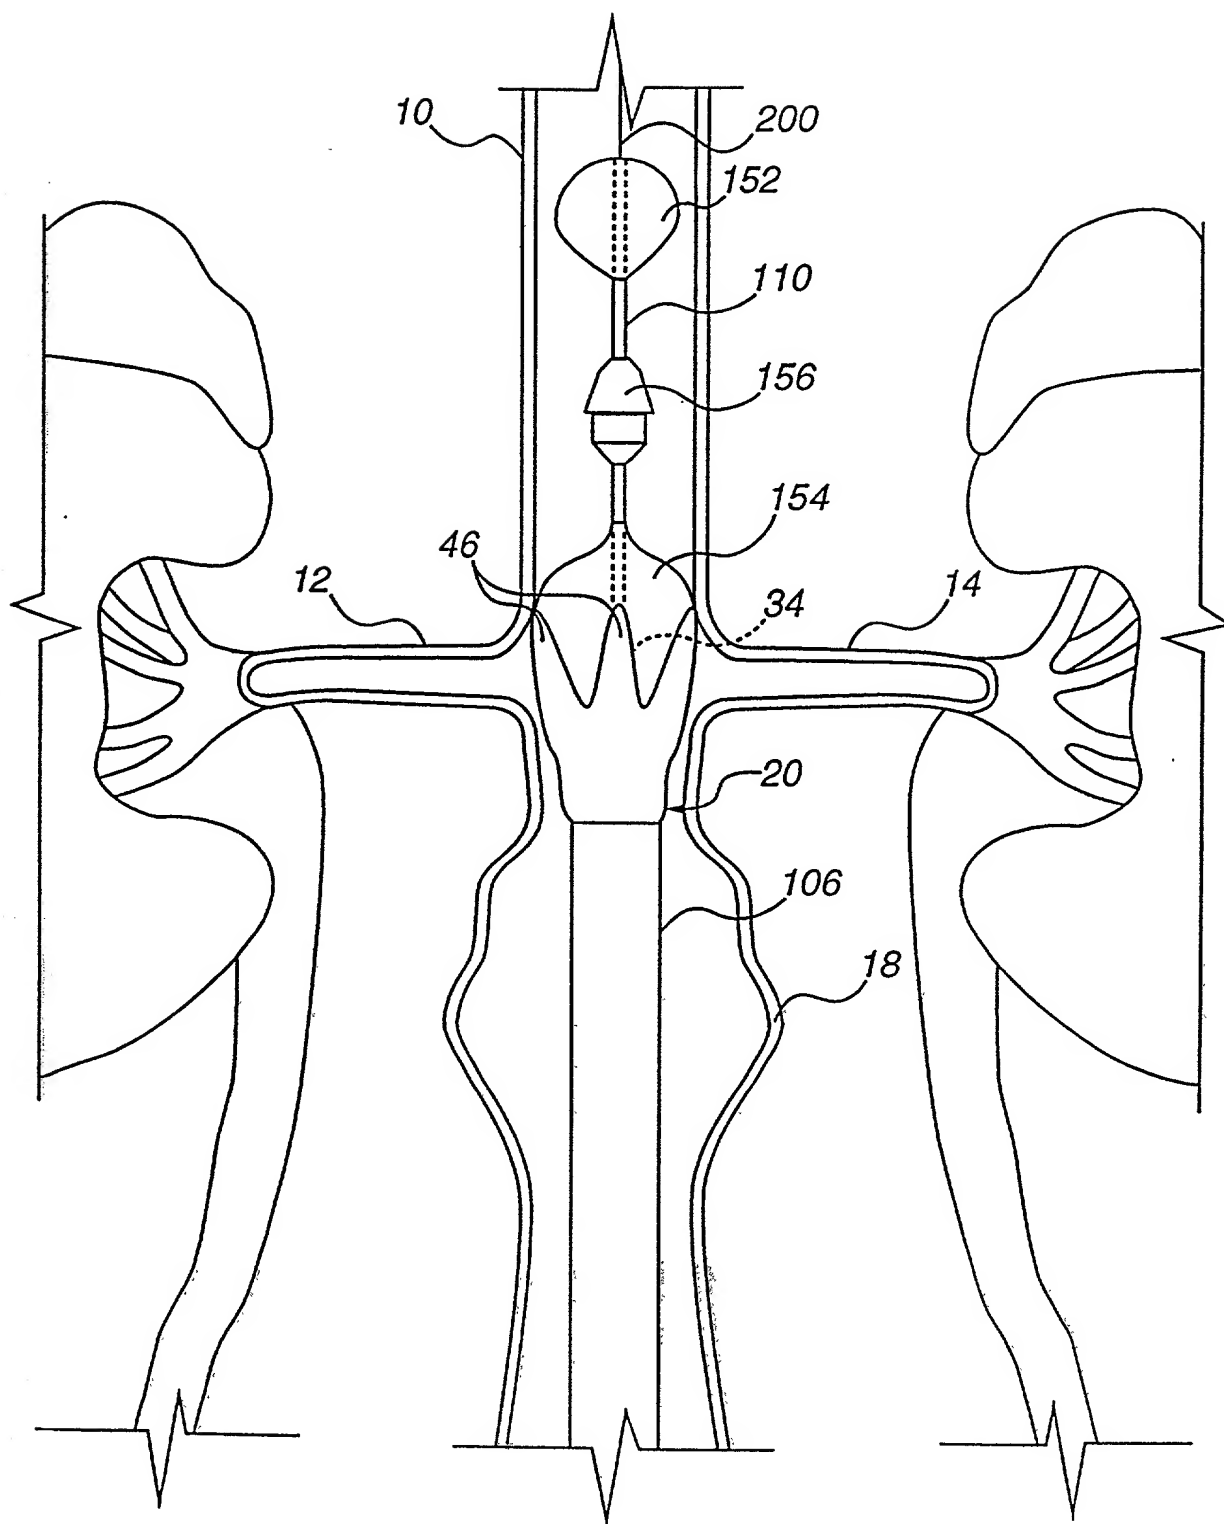


Fig. 9c

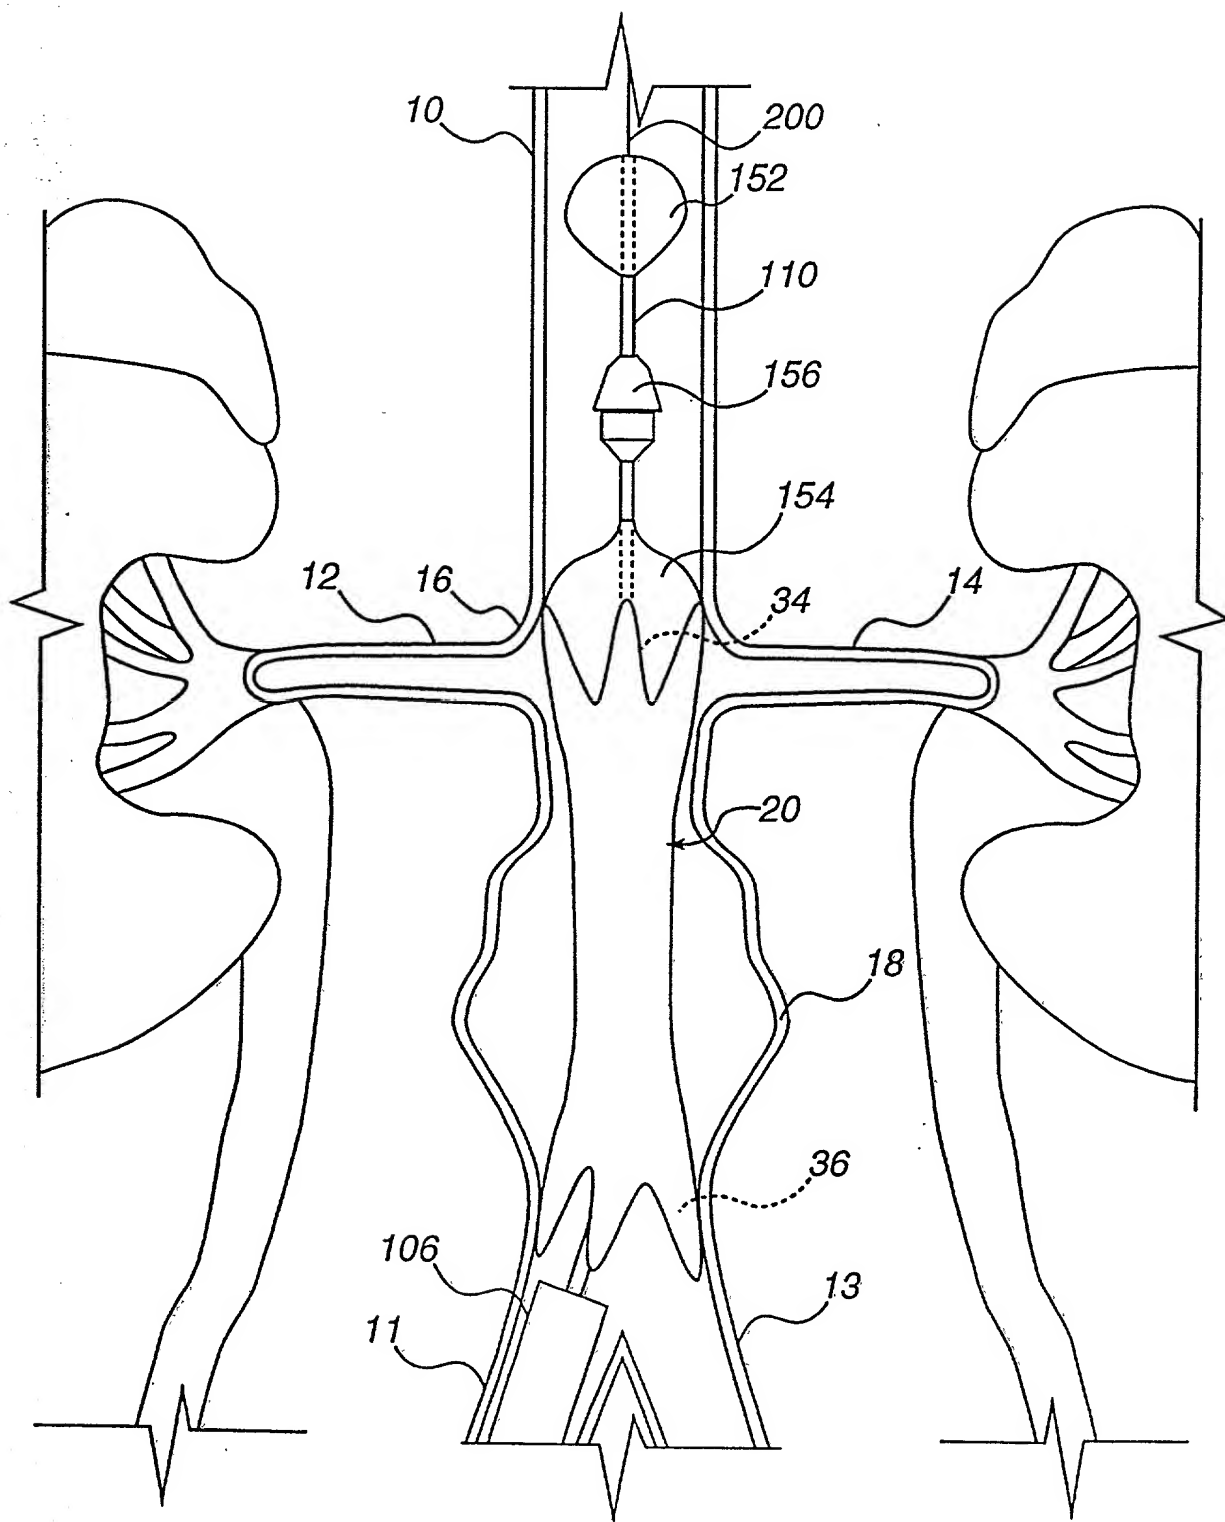


Fig. 9d

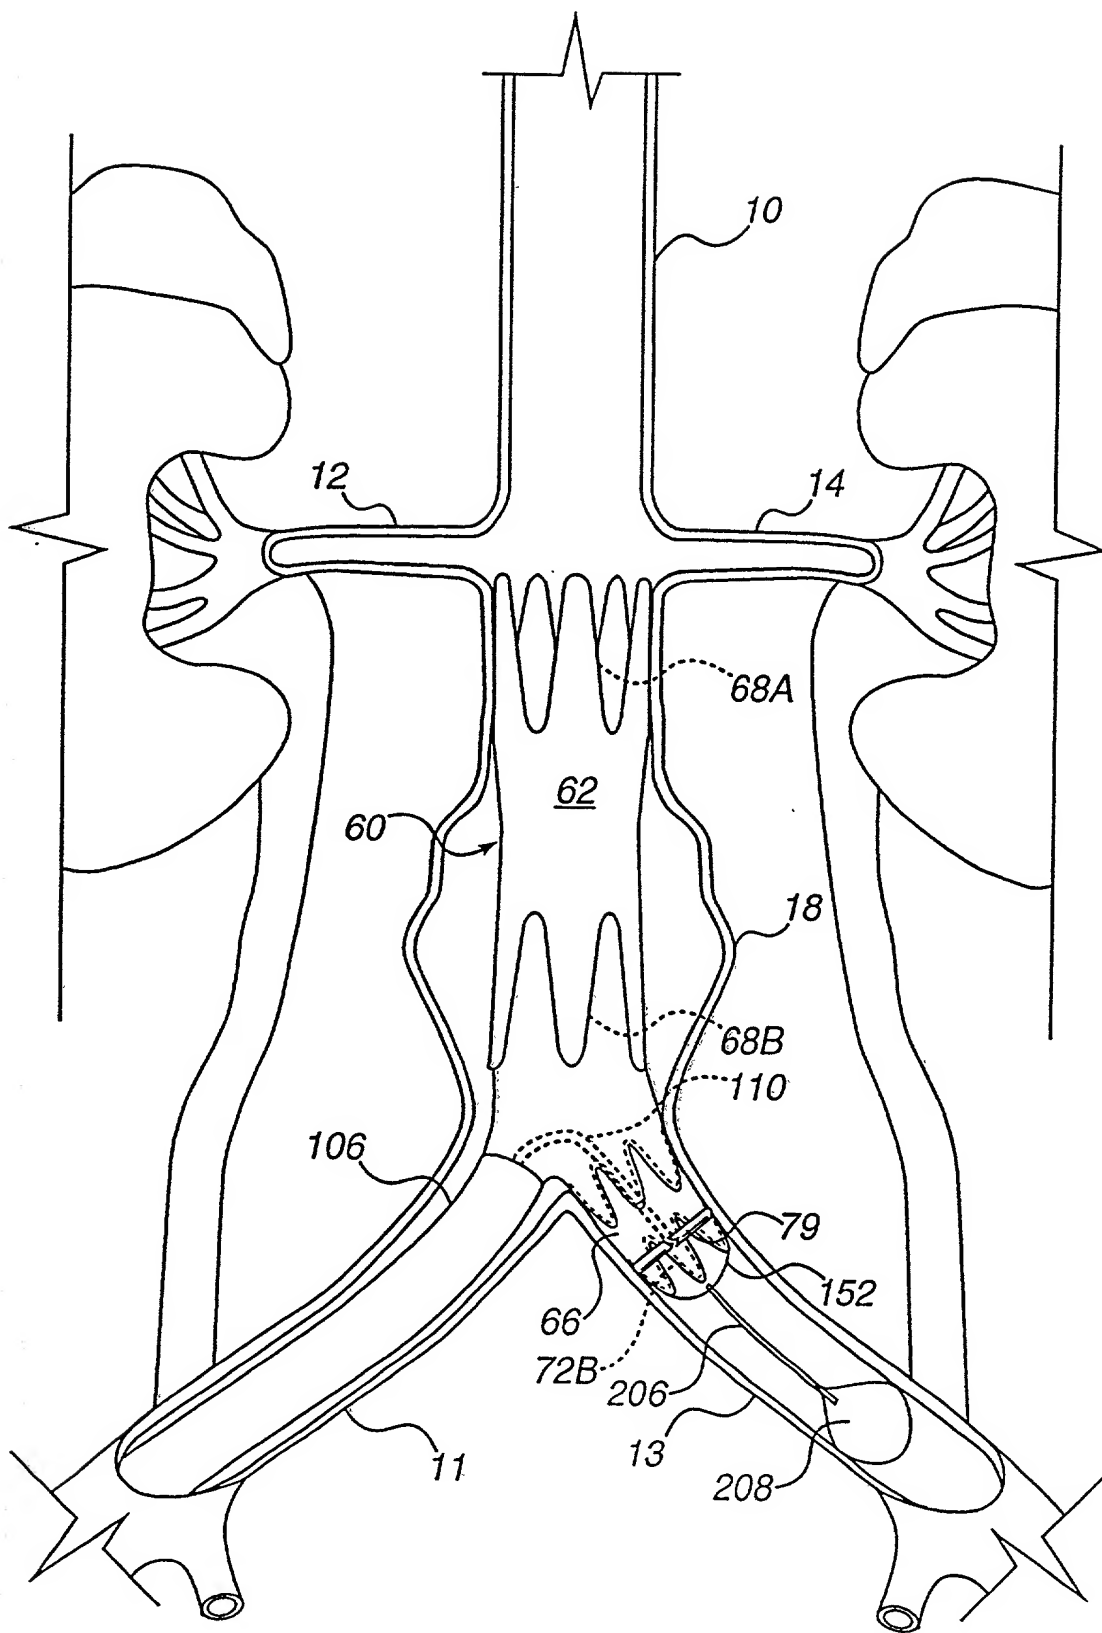


FIG. 10b

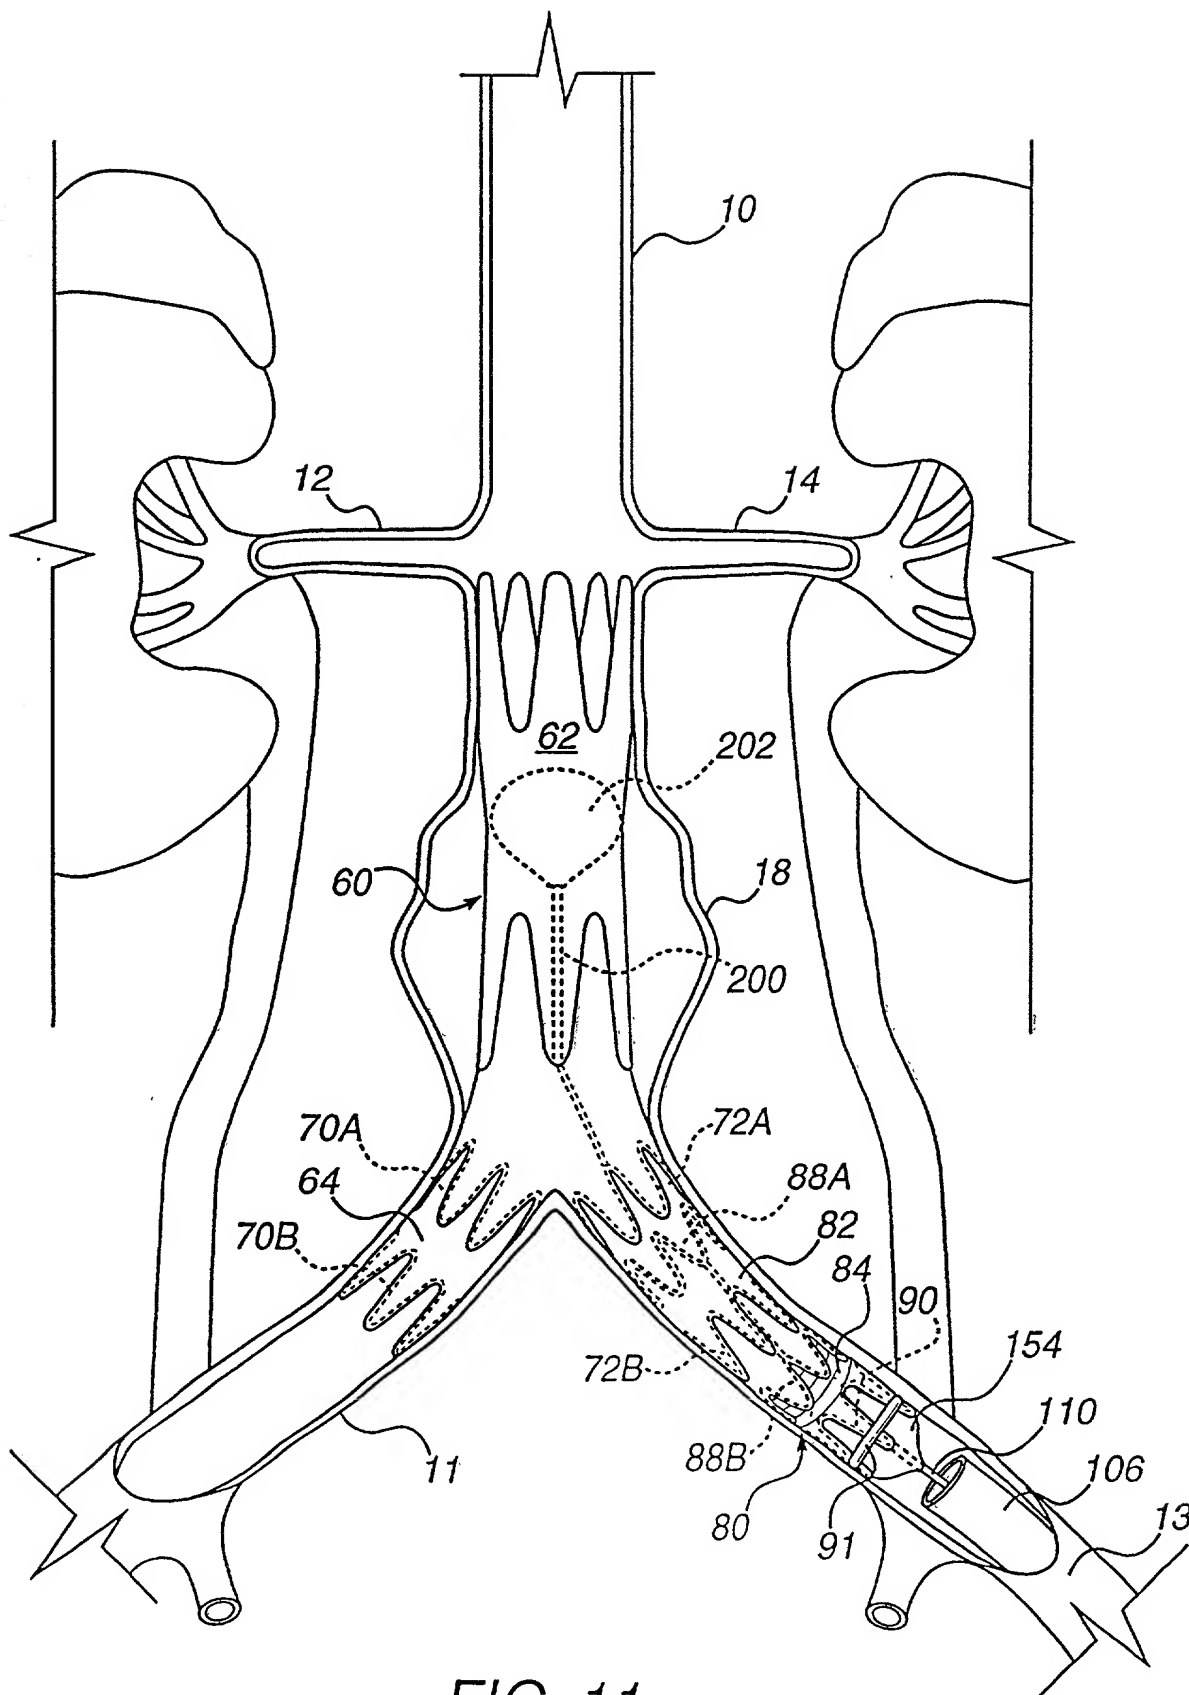


FIG. 11